

Hydrogen Sensor

SensoriC H2 3E 1%



SensoriC H2 3E 1%

FEATURES

Amperometric 3 electrode sensor cell
Fast response
Good long term stability

TYPICAL APPLICATIONS

Ambient monitoring
Very sensitive leak detection

PART NUMBER INFORMATION

MINI	0361-034-30009
SENSORIC CLASSIC	0361-034-30069
CTL 4 series adaptation	0361-034-30049
CTL 7 series adaptation	0361-034-30079

SensoriC deems the data contained herein as factual, and the opinions expressed are those of qualified experts based on the results of tests conducted. The above data can not be used as a warranty provision or representation for which SensoriC assumes legal responsibility. The data are offered solely for consideration, investigation and verification. Any use of this information is subject to federal, state and local laws and regulations.



Rev. 09/2006

SensoriC H2 3E 1%

TECHNICAL SPECIFICATIONS


Measuring Range	0–10000 ppm
Sensitivity Range	10 nA/ppm ± 5 nA/ppm
Zero Current at 20°C	< ± 250 nA
Resolution at 20°C	< 20 ppm
Bias Potential	0 V
Linearity	< 5% full scale
Response Time at 20°C	
t50	< 40 s calculated from 2 min. exposure time
t90	< 70 s calculated from 2 min. exposure time
Long Term Sensitivity Drift	< 10% per 6 months
Operation Conditions	
Temperature Range	-20°C to +40°C
Humidity Range	15–90% r.H., non–condensing
Effect of Humidity	no effect
Sensor Life Expectancy	> 24 months
Warranty	18 months

SensoriC deems the data contained herein as factual, and the opinions expressed are those of qualified experts based on the results of tests conducted. The above data can not be used as a warranty provision or representation for which SensoriC assumes legal responsibility. The data are offered solely for consideration, investigation and verification. Any use of this information is subject to federal, state and local laws and regulations.



SensoriC H2 3E 1%

OUTPUT vs. TEMPERATURE:

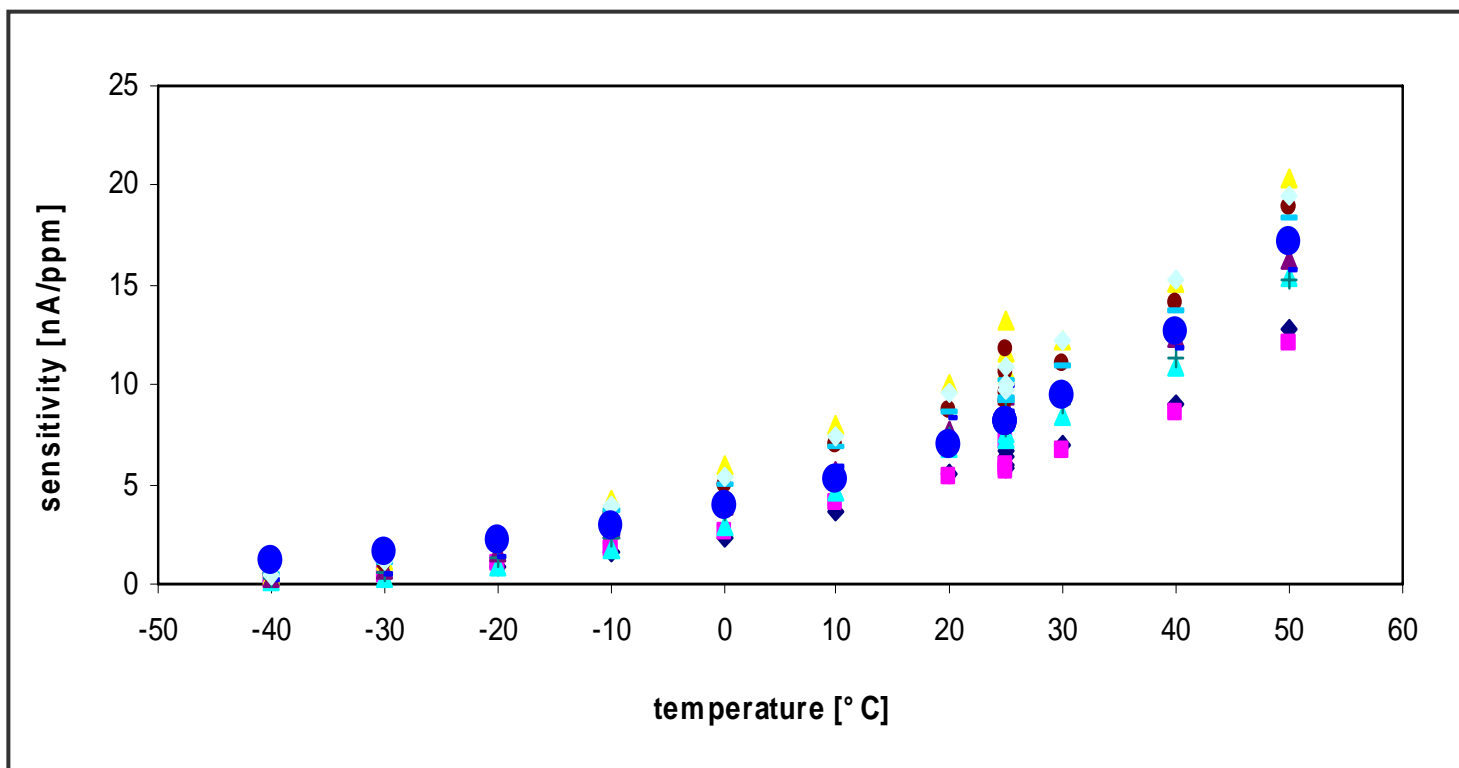


SensoriC deems the data contained herein as factual, and the opinions expressed are those of qualified experts based on the results of tests conducted. The above data can not be used as a warranty provision or representation for which SensoriC assumes legal responsibility. The data are offered solely for consideration, investigation and verification. Any use of this information is subject to federal, state and local laws and regulations.



Rev. 09/2006

SensoriC H2 3E 1%

ZERO READING vs. TEMPERATURE:

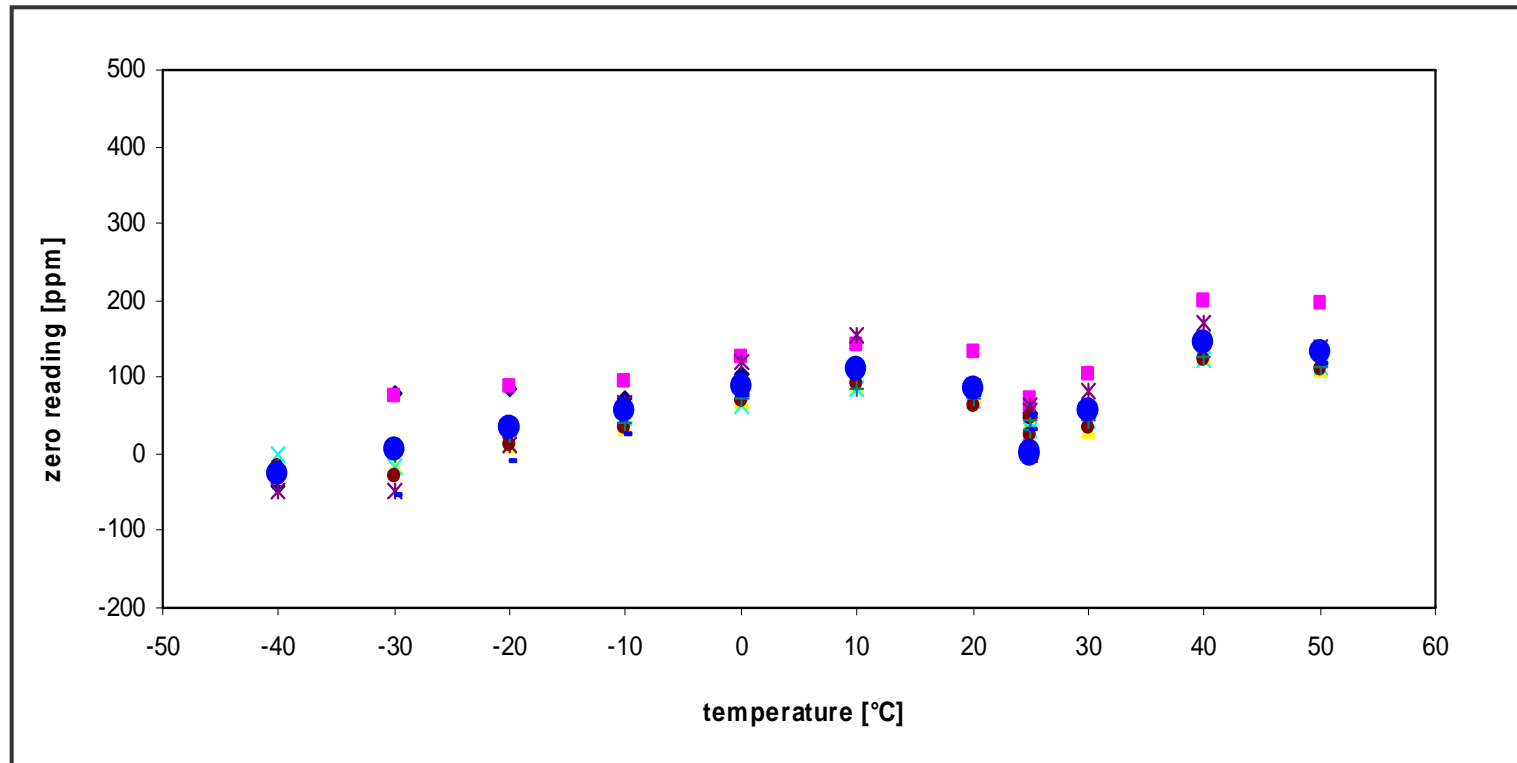

SensoriC deems the data contained herein as factual, and the opinions expressed are those of qualified experts based on the results of tests conducted. The above data can not be used as a warranty provision or representation for which SensoriC assumes legal responsibility. The data are offered solely for consideration, investigation and verification. Any use of this information is subject to federal, state and local laws and regulations.



Rev. 09/2006

SensoriC H2 3E 1%

CROSS SENSITIVITIES AT 20°C

Gas	Concentration	Reading [ppm]
Ammonia	100 ppm	0
Arsine	0.2 ppm	0
Carbon Dioxide	1000 ppm	0
Carbon Monoxide	100 ppm	150
Chlorine	1 ppm	0
Ethylene	500 ppm	yes; n/d
Hydrogen Cyanide	20 ppm	0
Hydrogen Sulfide	20 ppm	4 ¹
Isopropanol	1100 ppm	yes; n/d
Methane	1 %	0
Nitrogen Dioxide	10 ppm	-40
Ozone	0.25 ppm	0
Sulfur Dioxide	5 ppm	0

1) With inboard filter; to remove TLV levels of interfering gases; continuous high level exposure may reduce the efficiency of the filter material.

Notes:

1. Interference factors may differ from sensor to sensor and with life time. It is not advisable to calibrate with interference gases.
2. This table does not claim to be complete. The sensor might also be sensitive to other gases.

SensoriC deems the data contained herein as factual, and the opinions expressed are those of qualified experts based on the results of tests conducted. The above data can not be used as a warranty provision or representation for which SensoriC assumes legal responsibility. The data are offered solely for consideration, investigation and verification. Any use of this information is subject to federal, state and local laws and regulations.



Rev. 09/2006