




Carbon Dioxide Monitor Model 2166 3% CO₂

Features:

- Complete self contained units
- Non dispersive infrared (NDIR) technology
- Precision **low cost** gas cal. kit available
- Fast warm-up
- **Linear: 0-5 V** and **4-20 mA** outputs
- Dual level detect set points and relays
- **Yellow and Red** Limit Exceeded **Indicators**
- Cost effective - High quality
- Sample draw system with **pump switch** for calibration
- Solid state throughout - linear outputs
- Humidity and moisture resistant
- Dust-tight water resistant fiberglass enclosure
- **Digital readout** with 0.56 inch red LED display
- **Green Power** Indicator

Model 2166 3% CO₂

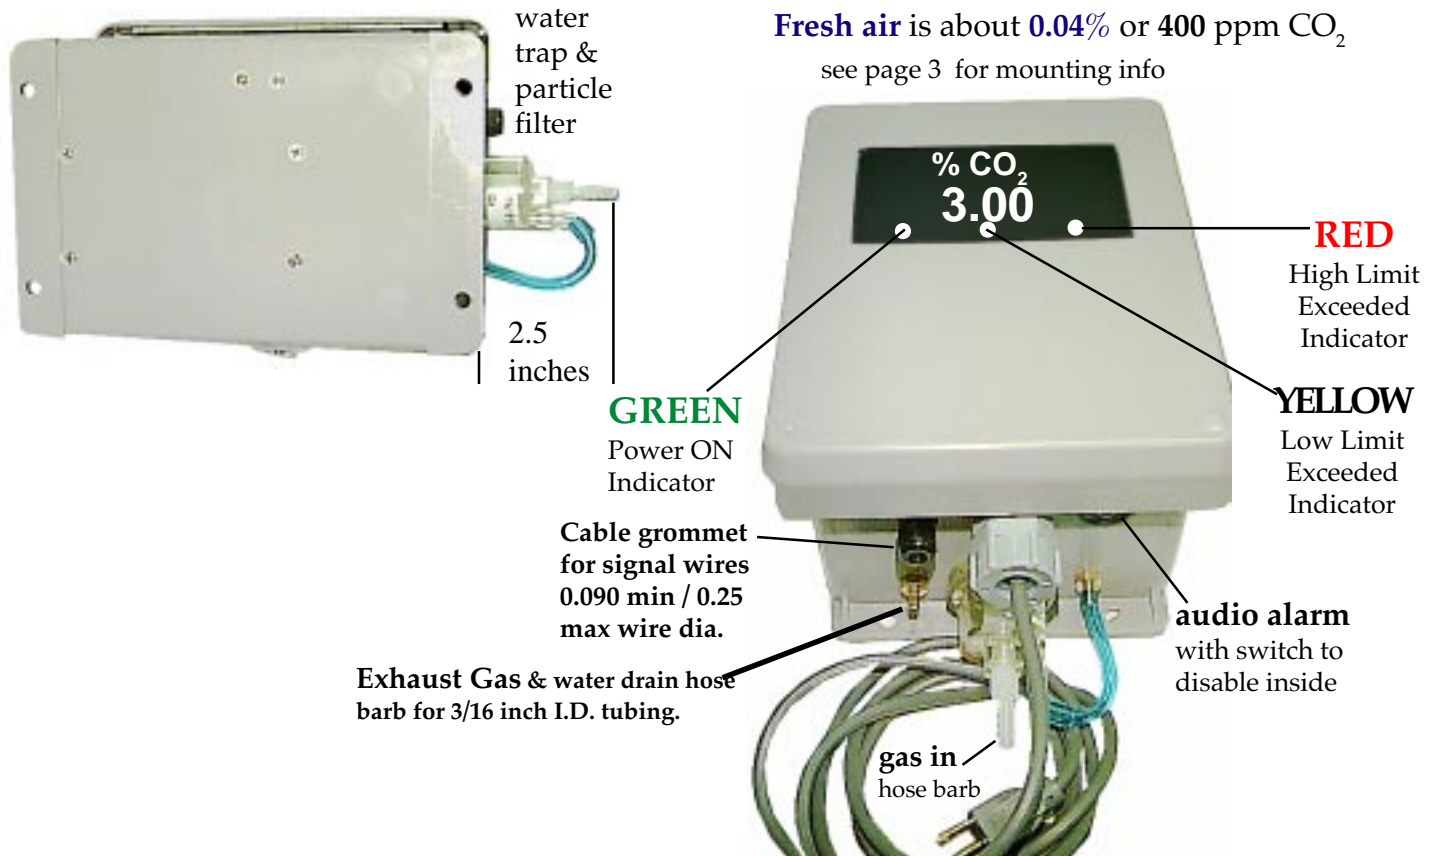

Overall Clearance: 5 x 7.5 x 13 inches including the water trap and 1/8" hose barb

Application:

- Industrial Safety
- Process Control
- Wineries
- Breweries
- Food Processing
- with CO₂ Blasters

The VALTRONICS Model 2166 is a non-dispersive infrared (NDIR) carbon dioxide monitor for use as an outdoor air sensor. It produces a control signal proportional to carbon dioxide concentration. This control signal is then used to provide remote control of the outdoor air dampers; thereby controlling the fresh air intake or varying the ventilation rates while maintaining safe indoor air quality. Dual adjustable level detect circuits may be used for alarms.



Carbon Dioxide Monitor Model 2166 3%

Description:

The Model 2166 is a non dispersive infrared gas monitor designed as a fully functioning stand-alone unit for the continuous monitoring of carbon dioxide. The optical system is not effected by humidity. The pumped gas sampling circuit has a self-draining water trap. This eliminates difficulties with water condensation in the sample lines. It has a 0.56 inch high digital readout and two adjustable level detect circuits with associated front panel indicators (yellow and red) and SPDT relay contacts.

This low power, water resistant system makes this an ideal remote sensor to interface with any central control unit. It has linear 0 to 5 volt and 4 to 20 mA current loop outputs. In either configuration, interfaced or stand-alone, this device is an excellent choice for any environment in which the level of carbon dioxide must be monitored or controlled.

Specifications: 2166 3% CO₂

Method: N.D. I. R. (Non-dispersive Infra-red) Gas sample pump (see **app note A67**)
 Gas: Carbon dioxide (CO₂)
 Range: 0-30,000 ppm (3.0%) CO₂
 Accuracy: ±0.075% CO₂ from 0 -1.5% CO₂ and ± 5% of reading from 1.5% to 3% CO₂
 Repeatability: ± 1% of full scale (challenge with same gas sample and assure zero)
 External Power Source: 115/220 VAC , 50/60 Hz
 Power Consumption: less than 8 watts @ 115 VAC
 Adjustable Set Points: Dual set points adjustable from 0.3% CO₂ to full scale (audio alarms below)
 Low SET Point adjusted to 0.5% and High SET Point to 2% unless specified on PO
 SET POINT Relay Contact Rating: ... SPDT contacts: non-latching N.C., N.O. 3 amp max. at 250 VAC or 30 VDC
 Display: 0.56 inch high digital Light Emitting Diode (LED) readout
 Output Signals:
 Voltage: 0 to 5 volt = 0 to 3% CO₂ (linear scale data attached)
 Current Loop: 4 to 20 mA = 0 to 3% CO₂ (linear scale data attached) 0 to 550Ω load
 Audio Alarms: Beeps once a second when Low SET Point is exceeded, continuous when High exceeded
 Set Point Indicators: Yellow flashes when Low SET Point is exceeded, RED on continuous when High exceeded
 Zero Drift at Constant Temperature: Less than 2% of full scale per month (random not cumulative)
 Zero Noise at Constant Temperature: Less than 50 mV peak to peak measured during any 20 second period
 measured on voltage output (equals less than 1% of full scale)
 Zero Drift due to Ambient Temperature: Less than 0.5% of full scale per degree Centigrade
 Operating Temperature Range: .. 0 to 50°C (32° to 122°F) see **Application Note A12**
 Storage Temperature Range: -40 to +70°C (-40 to +158°F)
 Operating Humidity Range: 5 to 95% RH (non-condensing) in gas cell, see **Application Note A30**
 Weight: Less than 6 pounds (< 2.72 kilograms)
 External Clearance Dimensions: . 5 inches high, 7.5 inches wide, 13 inches long (including 3.5" water trap)
 Mounting, four 0.312 inch dia holes ... Mounting centers 4.0 inch x 8.75 inch: see diagram

3463 Double Springs Road • Valley Springs, CA 95252 • (209) 754-0707 • FAX (209) 754-0104

e-mail: bpynenb@goldrush.com Model 2166 3% • Page 2 of 4 • Revised: **Feb 5, 2001**

SUNSTAR自动化 <http://www.sensor-ic.com/> TEL: 0755-83376489 FAX:0755-83376182 E-MAIL: szss20@163.com




Terminal block TB1 has a linear 0 to 5 volt output signal on pin number 9 with respect to pin number 8 which is signal common. Pin number 7 has a linear 4 to 20 mA current loop signal referenced again to pin number 8. See the wiring diagram on page 4.

The table below shows both the linear 0 to 5 volt and the 4 to 20 mA current loop responses to 0 to 3% carbon dioxide being drawn through the gas cell by the sample pump. The wires from TB1 go through the strain relief cable grommet shown on page 4. The resulting wire bundle must be between 0.090 and 0.25 inch diameter to be properly strain relieved.

VALTRONICS 3% Gas and 5 V full scale linear

±0.08% CO2				4-20 mA ±0.08% CO2			±10% of reading				4-20 mA ±10% of reading		
Gas in %	Output in volts	Max.	Min.	output	Max.	Min.	Gas in %	Output in volts	Max.	Min.	output	Max.	Min.
0.00	0.000	0.130	-0.130	4.00	4.40	3.60	1.55	2.583	2.713	2.454	12.27	12.68	11.85
0.05	0.083	0.213	-0.047	4.27	4.67	3.87	1.60	2.667	2.800	2.533	12.53	12.96	12.11
0.10	0.167	0.297	0.037	4.53	4.93	4.13	1.65	2.750	2.888	2.613	12.80	13.24	12.36
0.15	0.250	0.380	0.120	4.80	5.20	4.40	1.70	2.833	2.975	2.692	13.07	13.52	12.61
0.20	0.333	0.463	0.203	5.07	5.47	4.67	1.75	2.917	3.063	2.771	13.33	13.80	12.87
0.25	0.417	0.547	0.287	5.33	5.73	4.93	1.80	3.000	3.150	2.850	13.60	14.08	13.12
0.30	0.500	0.630	0.370	5.60	6.00	5.20	1.85	3.083	3.238	2.929	13.87	14.36	13.37
0.35	0.583	0.713	0.453	5.87	6.27	5.47	1.90	3.167	3.325	3.008	14.13	14.64	13.63
0.40	0.667	0.797	0.537	6.13	6.53	5.73	1.95	3.250	3.413	3.088	14.40	14.92	13.88
0.45	0.750	0.880	0.620	6.40	6.80	6.00	2.00	3.333	3.500	3.167	14.67	15.20	14.13
0.50	0.833	0.963	0.703	6.67	7.07	6.27	2.05	3.417	3.588	3.246	14.93	15.48	14.39
0.55	0.917	1.047	0.787	6.93	7.33	6.53	2.10	3.500	3.675	3.325	15.20	15.76	14.64
0.60	1.000	1.130	0.870	7.20	7.60	6.80	2.15	3.583	3.763	3.404	15.47	16.04	14.89
0.65	1.083	1.213	0.953	7.47	7.87	7.07	2.20	3.667	3.850	3.483	15.73	16.32	15.15
0.70	1.167	1.297	1.037	7.73	8.13	7.33	2.25	3.750	3.938	3.563	16.00	16.60	15.40
0.75	1.250	1.380	1.120	8.00	8.40	7.60	2.30	3.833	4.025	3.642	16.27	16.88	15.65
0.80	1.333	1.463	1.203	8.27	8.67	7.87	2.35	3.917	4.113	3.721	16.53	17.16	15.91
0.85	1.417	1.547	1.287	8.53	8.93	8.13	2.40	4.000	4.200	3.800	16.80	17.44	16.16
0.90	1.500	1.630	1.370	8.80	9.20	8.40	2.45	4.083	4.288	3.879	17.07	17.72	16.41
0.95	1.583	1.713	1.453	9.07	9.47	8.67	2.50	4.167	4.375	3.958	17.33	18.00	16.67
1.00	1.667	1.797	1.537	9.33	9.73	8.93	2.55	4.250	4.463	4.038	17.60	18.28	16.92
1.05	1.750	1.880	1.620	9.60	10.00	9.20	2.60	4.333	4.550	4.117	17.87	18.56	17.17
1.10	1.833	1.963	1.703	9.87	10.27	9.47	2.65	4.417	4.638	4.196	18.13	18.84	17.43
1.15	1.917	2.047	1.787	10.13	10.53	9.73	2.70	4.500	4.725	4.275	18.40	19.12	17.68
1.20	2.000	2.130	1.870	10.40	10.80	10.00	2.75	4.583	4.813	4.354	18.67	19.40	17.93
1.25	2.083	2.213	1.953	10.67	11.07	10.27	2.80	4.667	4.900	4.433	18.93	19.68	18.19
1.30	2.167	2.297	2.037	10.93	11.33	10.53	2.85	4.750	4.988	4.513	19.20	19.96	18.44
1.35	2.250	2.380	2.120	11.20	11.60	10.80	2.90	4.833	5.075	4.592	19.47	20.24	18.69
1.40	2.333	2.463	2.203	11.47	11.87	11.07	2.95	4.917	5.163	4.671	19.73	20.52	18.95
1.45	2.417	2.547	2.287	11.73	12.13	11.33	3.00	5.000	5.250	4.750	20.00	20.80	19.20
1.50	2.500	2.630	2.370	12.00	12.40	11.60							

Accuracy = ±0.075% CO2 from 0 to 1.5% CO2 and ±5% of reading from 1.5 to 3% CO2
Chart Revised on 3-5-97

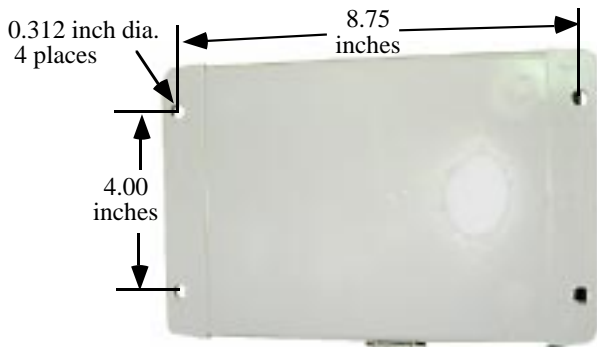

Rear view:



Signal and relay wires pass through this strain relief cable grommet.



Cable grommet for signal wires
0.090 min / 0.25 max wire dia.

Cable grommet for
AC power cord

Audio
Alarm

Exhaust Gas
and water
drain hose
barb for 3/16
inch I.D.
tubing

Gas Inlet
hose barb
for 1/4 inch
I.D. tubing

Water Trap

JP2



JP1

Caution: Note jumper configuration for either **115 VAC** (JP1 & JP2) or **230 VAC** (JP3 only) operation.

Preventive Maintenance:

Gas calibration should be done every six months. At least calibration with zero gas (nitrogen) every six months and both zero and span (certified 1% or 2% CO₂) at least once a year. A calibration log book where you record how much ZERO and SPAN had drifted before it was recalibrated will help you decide what the optimum duration between calibrations should be. See **Application Note A24 & A73** for detailed calibration instructions. The **pump switch** should be **turned off** during gas calibration and the flow rate set to about 1 to 2 Liters per minute. The filter in the water trap and the hydrophobic / particle filter inside should be inspected and changed when necessary. The flow rate of the pump should be checked to see if it is still operating properly. It should be about 3 to 5 liters per minute if measured at the water trap input, Gas Inlet (both sides of the pump drawing). See **Application Note A67** for spare parts information. See **Application Note A46** for detailed info on PC board.

Terminal Block TB1


High Level SET POINT Adj. R48

S1 Level detect adjust select

Low Level SET POINT Adj. R44

SPAN
Adjust

ZERO
Adjust

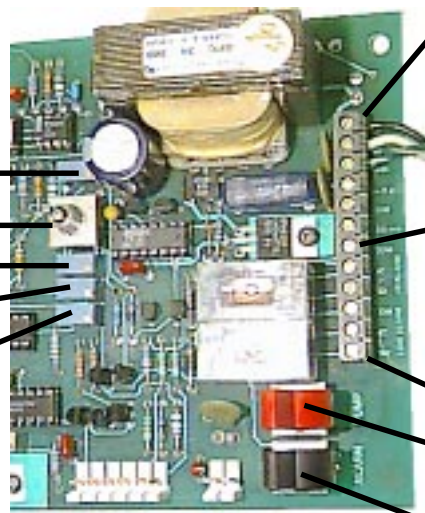

- 12. AC power High
- 11. AC power neutral
- 10. Earth Ground
- 9. 0 to 5 volt signal out
- 8. Signal common
- 7. 4-20 mA current loop out
- 6. High Alarm Common (relay contact)
- 5. High Alarm N.C. (relay contact)
- 4. High Alarm N.O. (relay contact)
- 3. Low Alarm Common (relay contact)
- 2. Low Alarm N.C. (relay contact)
- 1. Low Alarm N.O. (relay contact)

Pump
Switch
Alarm
Switch