


# Technical Specification

## CL2-B1 Chlorine Sensor



Figure 1 CL2-B1 Schematic Diagram

PATENTED

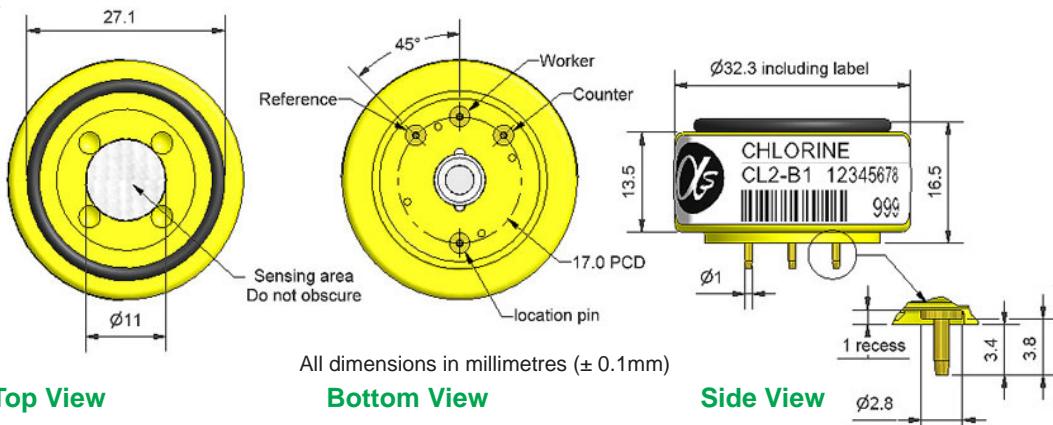

<b>PERFORMANCE</b>	Sensitivity	nA/ppm in 10ppm Cl <sub>2</sub>	-600 to -950
	Response time	t <sub>90</sub> (s) from zero to 10ppm Cl <sub>2</sub> (33Ω load resistor)	< 60
	Zero current	ppm equivalent in zero air	± 0.2
	Resolution	RMS noise (ppm equivalent) (33Ω load resistor)	< 0.02
	Range	ppm limit of performance warranty	20
	Linearity	ppm error at full scale, linear at zero and 10ppm Cl <sub>2</sub>	<± 0.2
	Oversaturation limit	maximum ppm for stable response to gas pulse	60
<b>LIFETIME</b>	Zero drift	ppm equivalent change/year in lab air	< 0.03
	Sensitivity drift	% change/year in lab air, monthly test	< 6
	Operating life	months until 80% original signal (24 month warranted)	> 24
<b>ENVIRONMENTAL</b>	Sensitivity	@ -20°C% (output @ -20°C/output @ 20°C) @ 10ppm	80 to 93
	Sensitivity	@ 50°C% (output @ 50°C/output @ 20°C) @ 10ppm	99 to 109
	Zero @ -20°C	ppm equivalent change from 20°C	0 to +0.3
	Zero @ 50°C	ppm equivalent change from 20°C	<± 0.2
	Zero slope	equivalent ppm/K	-0.003
<b>CROSS SENSITIVITY</b>	H <sub>2</sub> S	sensitivity % measured gas @ 20ppm	-100
	NO <sub>2</sub>	sensitivity % measured gas @ 10ppm	100
	NO	sensitivity % measured gas @ 50ppm	< 0.5
	SO <sub>2</sub>	sensitivity % measured gas @ 20ppm	< -2
	CO	sensitivity % measured gas @ 400ppm	< 0.1
	H <sub>2</sub>	sensitivity % measured gas @ 400ppm	< 0.1
	C <sub>2</sub> H <sub>4</sub>	sensitivity % measured gas @ 400ppm	< 0.1
	NH <sub>3</sub>	sensitivity % measured gas @ 20ppm	< 0.1
	CO <sub>2</sub>	sensitivity % measured gas @ 5% (Vol)	0
<b>KEY SPECIFICATIONS</b>	Temperature range	°C	-20 to 50
	Pressure range	kPa	80 to 120
	Humidity range	% rh continuous (see note below)	15 to 90
	Storage period	months @ 3 to 20°C (stored in sealed pot)	6
	Load resistor	Ω (for optimum performance)	33
	Weight	g	< 13

Note: Above 85% rh and 40°C a maximum continuous exposure period of 10 days is warranted. Where such exposure occurs the sensor will recover normal electrolyte volumes when allowed to rest at lower % rh and temperature levels for several days.



NOTE: all sensors are tested at ambient environmental conditions, with 10 ohm load resistor, unless otherwise stated. As applications of use are outside our control, the information provided is given without legal responsibility. Customers should test under their own conditions, to ensure that the sensors are suitable for their own requirements.

# Technical Specification

## CL2-B1 Performance Data

Figure 2 Sensitivity Temperature Dependence

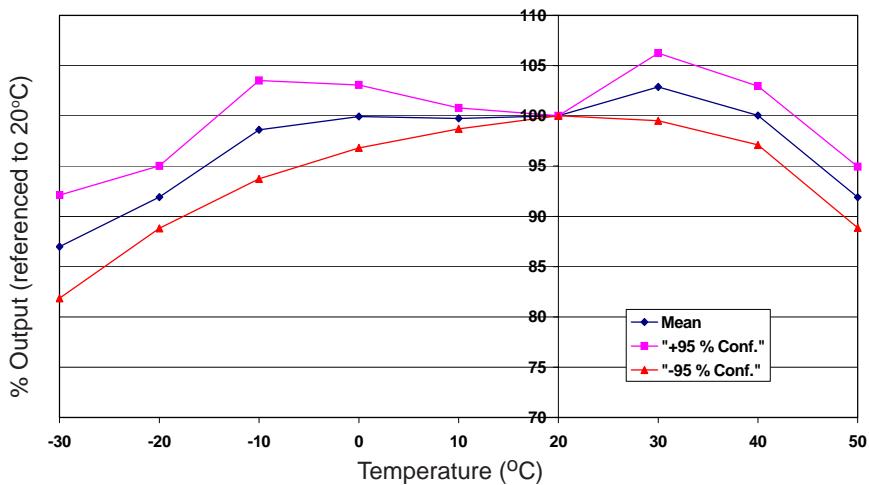


Figure 2 shows the variation in sensitivity caused by changes in temperature.

This data is taken from a typical batch of sensors. The mean and  $\pm 95\%$  confidence intervals are shown

Chlorine gas tests can be difficult and non-repeatable, especially at higher temperature.

Figure 3 Zero Temperature Dependence

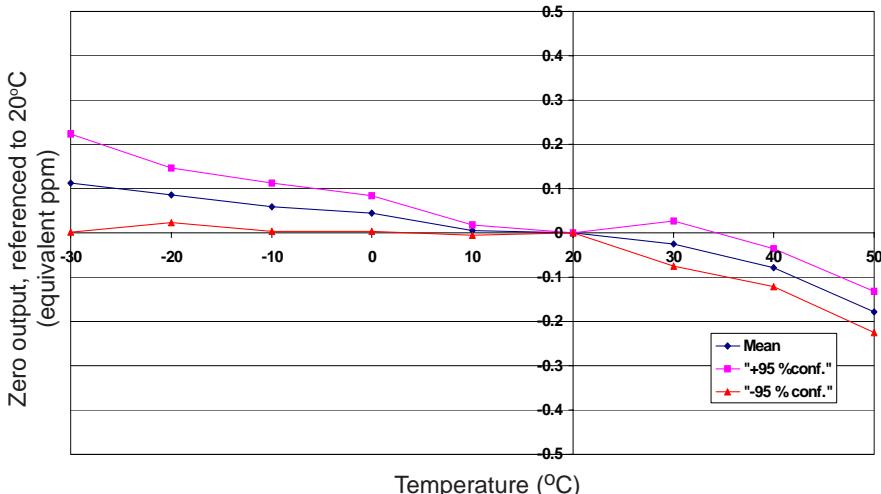


Figure 3 shows the variation in zero output caused by changes in temperature expressed as ppm gas equivalent.

This data is taken from a typical batch of sensors. The mean and  $\pm 95\%$  confidence intervals are shown.

Figure 4 Effects of Changes in Relative Humidity (rh)

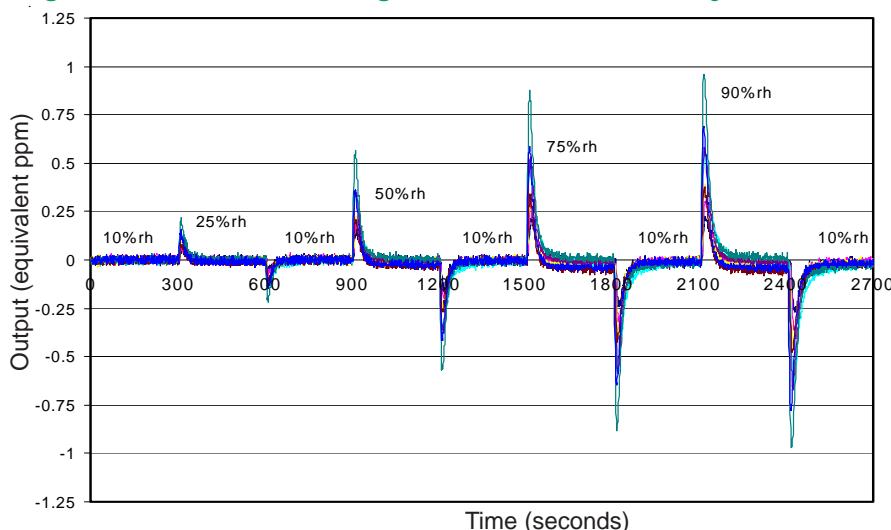


Figure 4 shows the effect on zero with increasing step changes of relative humidity of 25%rh, 50%rh, 75%rh and 95%rh.

The relative humidity level is returned to 10% between each upward going exposure.

This sensor provides an exceptionally low transient response to large step changes in relative humidity.